


Proposed divertor SPRED fiberoptic bundle routing and CCD detector placement

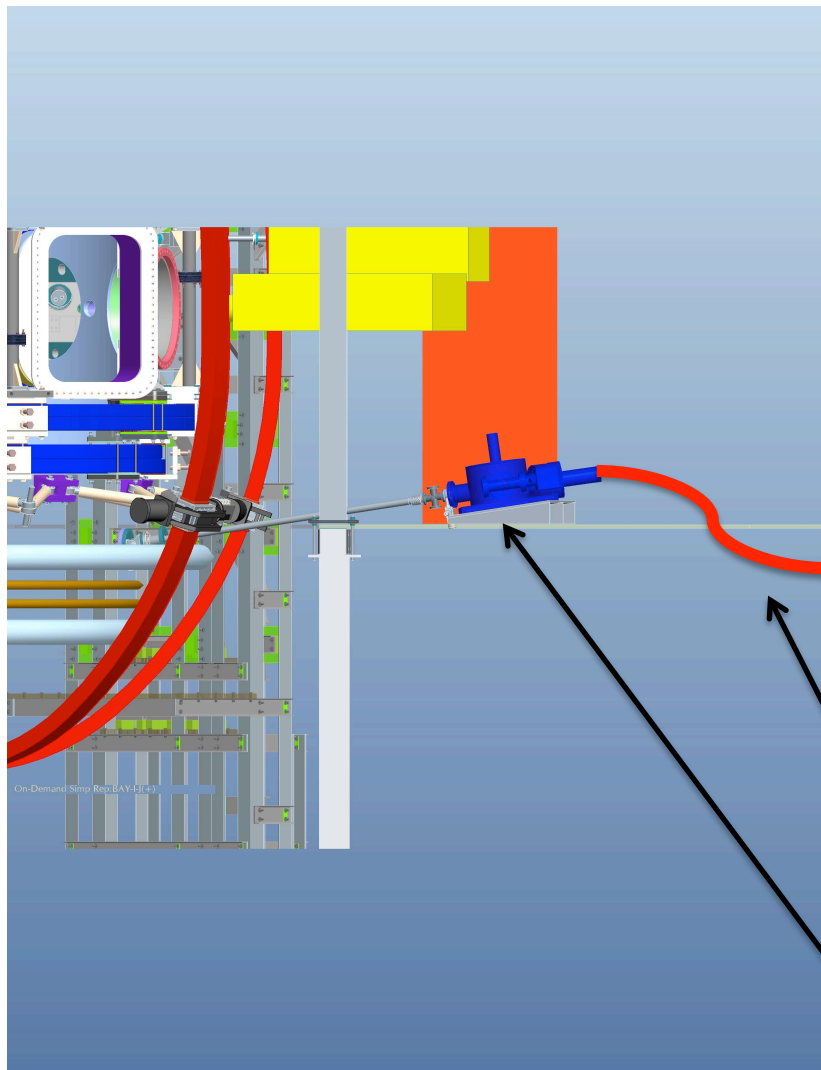

109' elevation floor

CCD detector on shelf
suspended under floor

12.5' semi-rigid fiberoptic
bundle in kor-lok

Divertor SPRED

**Motivation: need to remove CCD detector as far away from machine
(magnetic field) as possible**